# Field Service Bulletin No. 17

Order No.: DD+DIS223.01E
1 piece UQHD5 MA1

## ADC Solo
Type 5155 / 100

## Path Speed CR SP1001
Type 5155 / 200

| Rating | | | When? | | |
|---|---|---|---|---|---|
| safety relevant | reliability | new function | immediately | next service | as required |
| | | X | | | X |

Please file this document in section 13 of your technical documentation

# New ADC Cassettes for Mammo and Asymmetric Scanning introduced

## List of Contents

1 General ..... 2
1.1 Software Requirements ..... 2
2 Short Description of the ADC Mammo Cassette .... 2
3 Short Description of the ADC Cassette for Asymmetric Scanning ..... 3

printed in Germany 09 / 2001

AGFA

# 1 General

Two new types of ADC Cassettes are introduced:

- ADC Mammo Cassette for implant imaging
- ADC Cassette for asymmetric scanning

## 1.1 Software Requirements

| | |
|---|---|
| ADC Compact Digitizer: | ≥ COP_1308 |
| ADC Solo Digitizer: | ≥ SOL_1213 |
| PRID Software: | ≥ 1.2.09 |
| CCM tool: | ≥ 1.1.06 |

# 2 Short Description of the ADC Mammo Cassette

The ADC Mammo Cassette is only foreseen for mammography of breast implants and must not be used for other mammographic applications or diagnostics!

**Identification:**
The cassette is labeled with “Mammo” on both sides and with “Implants” on the tube side.
The cassette is preinitialised as a Mammo Cassette, but if the identification is lost, it can be given via the ID Station.

**Formats:**
The ADC Mammo Cassette is available in two formats:

- 18 cm x 24 cm
- 24 cm x 30 cm

**Specification:**
The ADC Mammo Cassette contains normally a regular ADC MD30 image plate. This type of image plate has a special phosphor layer which results in a high dynamic range. The cassette is equipped with a special hinge in order to reduce the chest wall distance to the image plate.

The Mammo Cassette is intended to follow up implants (silicone, prosthesis) to check for position, leaks or calcifications.

## 3 Short Description of the ADC Cassette for Asymmetric Scanning

**Identification:**

A Cassette for asymmetric scanning can be identified by a red hatching covering less than the half of the cassette side. (see Figure 1)

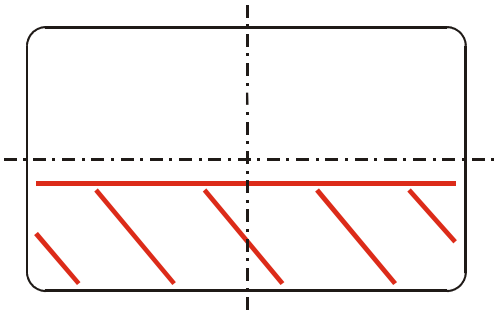

Figure 1

**Formats:**
The ADC Asymmetric Cassette is available in:

- 21 cm x 43 cm (asymmetric partial scan of dedicated 35 x 43 cassettes)

**Specification:**
The Asymmetric Cassette is dedicated for X-ray exposures where no centered positioning of the part of the body is possible (e.g. side view of a spinal column).